

Physician: Sample

Assay Batch #: G0617a08

Patient: Sample

Collected: 06/04/08


Accession #:

Received: 06/05/08

Age: 6

Completed: 06/18/08

Sex: F

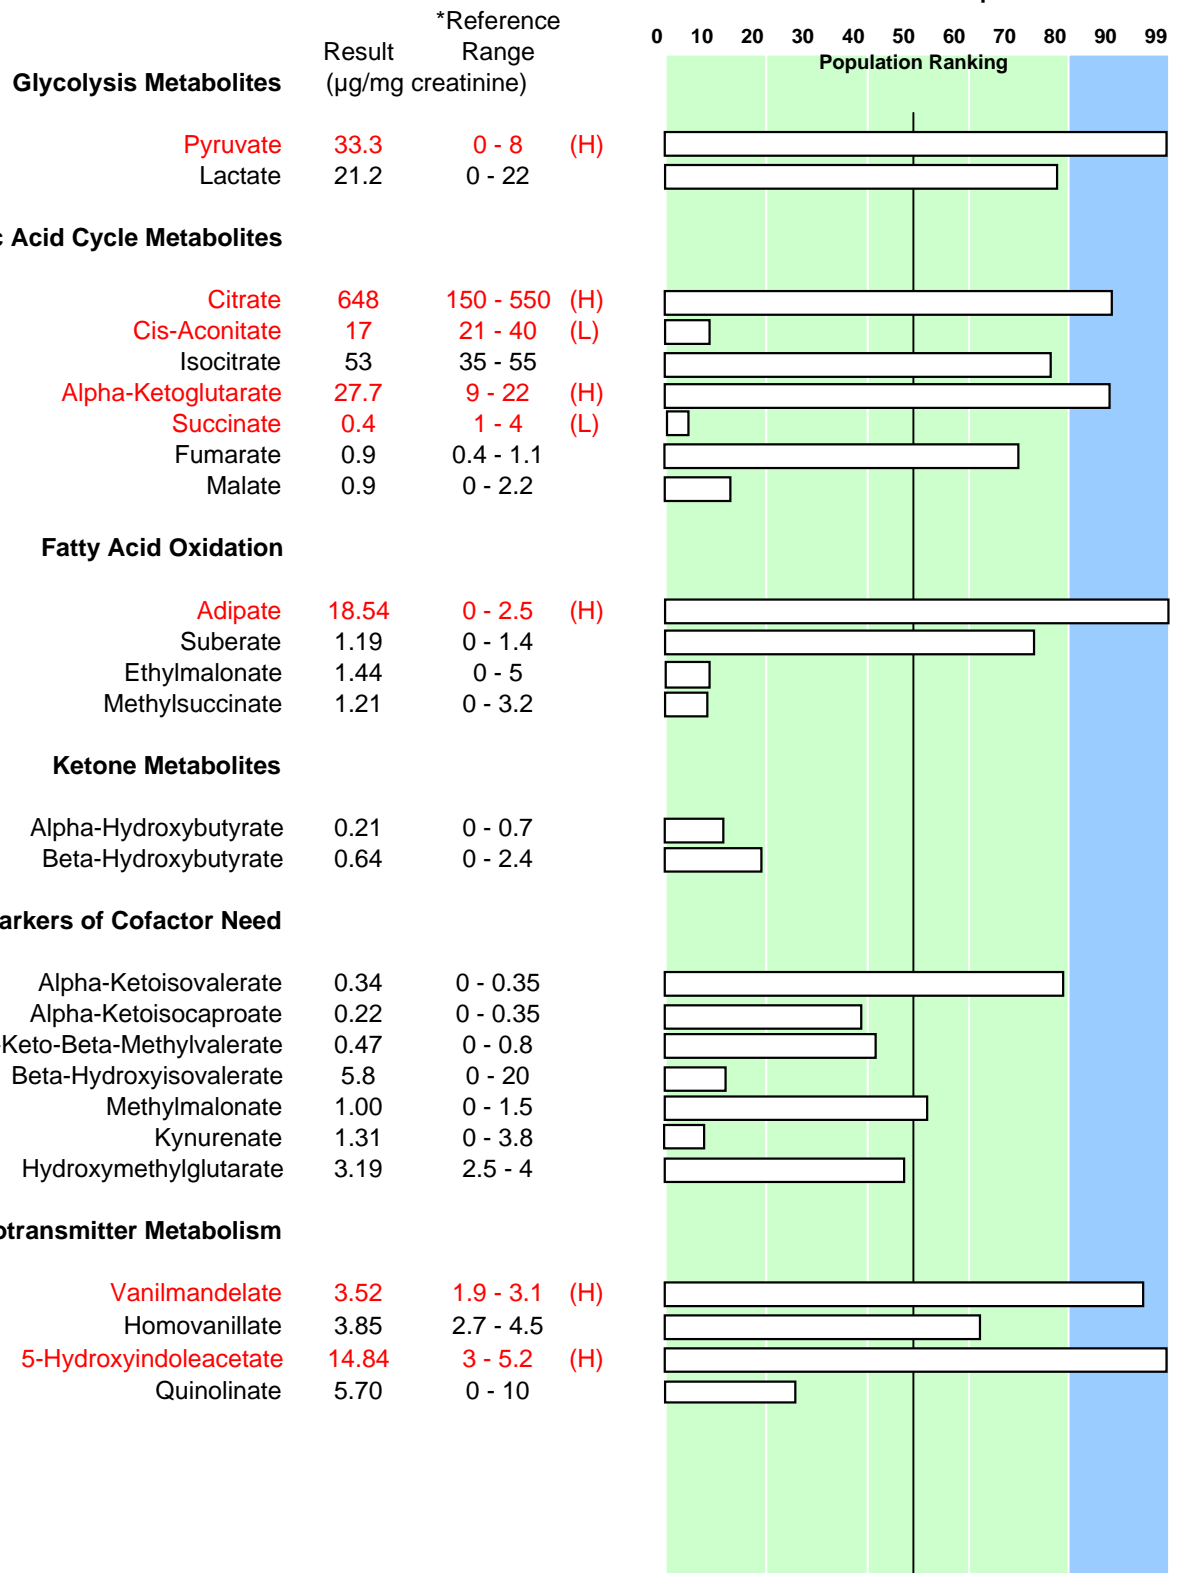


\*Reference ranges are gender specific and results are age adjusted for children

MEAN

**Physician:** Sample  
**Patient:** Sample  
**Accession #:**  
**Age:** 6  
**Sex:** F

Assay Batch #: G0617a08  
**Collected:** 06/04/08  
**Received:** 06/05/08  
**Completed:** 06/18/08  
 Reference Updated as of 02/08/05  
 Report format updated 01/28/08

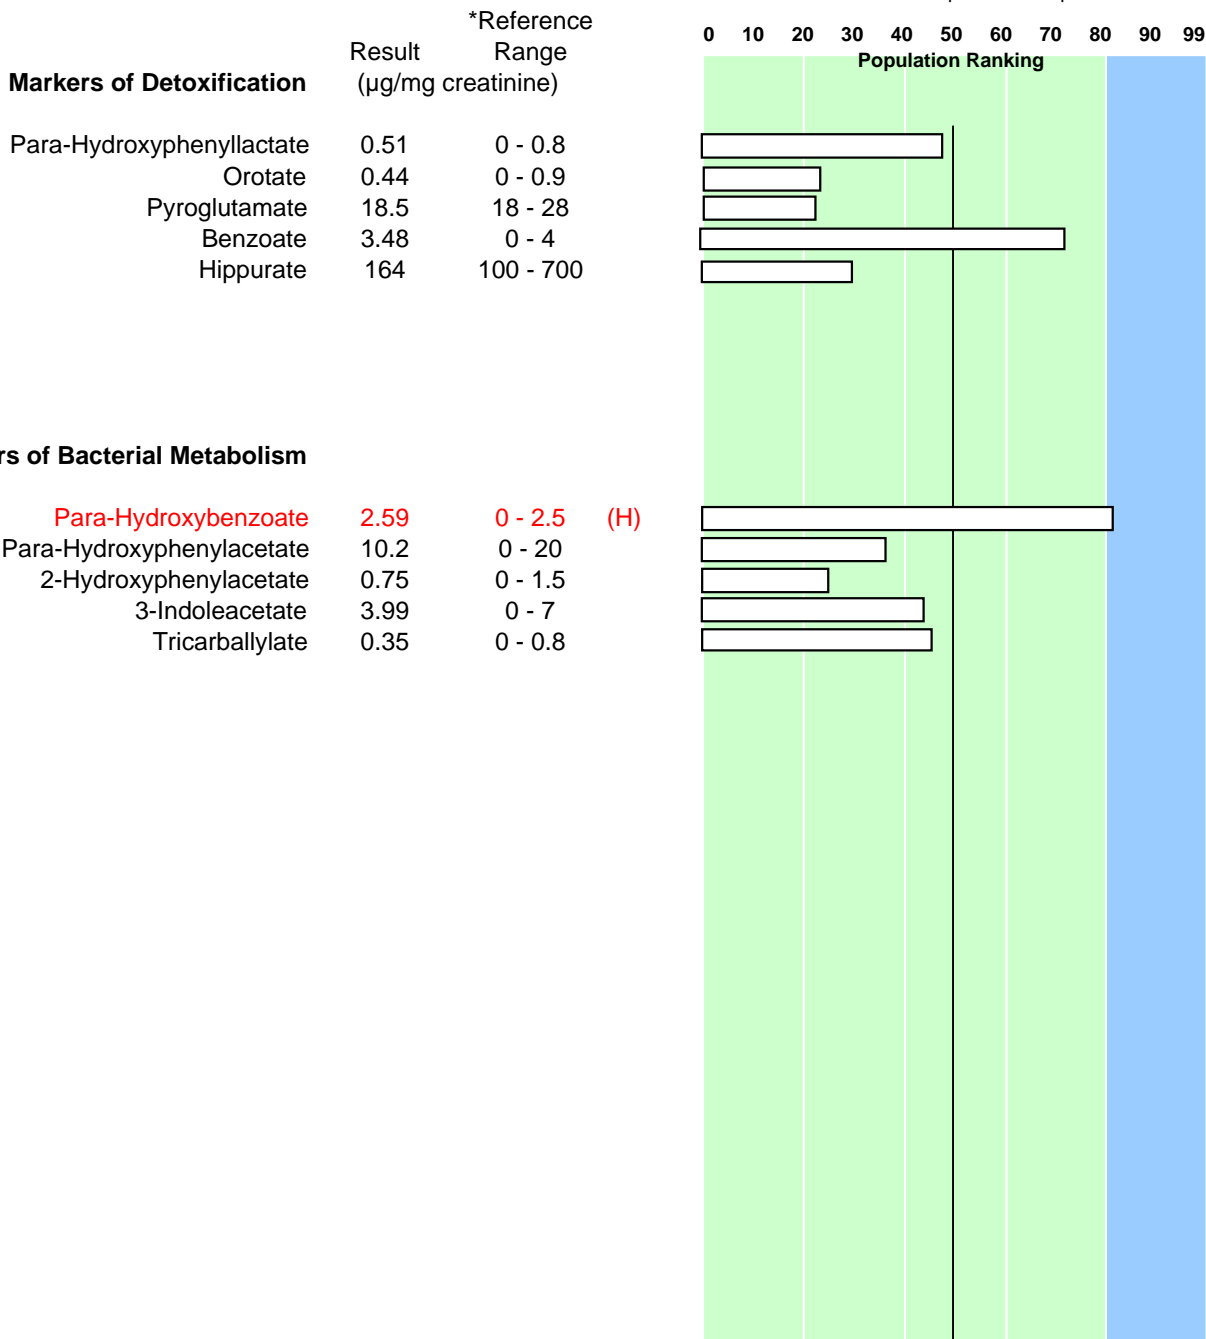

The analytes on the panel are subject to change without prior notice

MEAN

\*Reference ranges are gender specific and results are age adjusted for children

CLIA #: 50DO965661

© US BioTek 2005

US BioTek Laboratories has developed and determined the performance characteristics of this test.

This test has not been evaluated by the U.S. Food and Drug Administration.

This test does not assess for neonatal inborn errors of metabolism and is based on stable renal function and normal renal clearance.